



## Instructions for Use Reprocessed Visions PV .035 Digital IVUS Catheter

### Reprocessed Device for Single Use

**Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.**

### DEVICE DESCRIPTION

The Reprocessed Visions PV .035 catheter is an over-the-wire intravascular imaging catheter with a digital ultrasound transducer at the distal end. The transducer utilizes a 64-element cylindrical array that radiates acoustic energy into the surrounding tissue and detects the subsequent echoes. The information from the echoes is used to generate real-time images of the peripheral vessels.

The catheter is introduced percutaneously or via surgical cutdown into the vascular system, and it is designed to track over 0.035"-.038" (0.89-0.97mm) guide wires.

The catheter has body markers 1 cm apart along the working length. There are 25 radiopaque markers on the distal end of the catheter, starting 1cm from the imaging plane, with the 25<sup>th</sup> RO marker overlapping the distal most wide inked marker. Inked markers (non-radiopaque) continue along the shaft, spaced 1 cm apart, middle-to-middle, with wider marks indicating 5 cm intervals (See Figure 1).

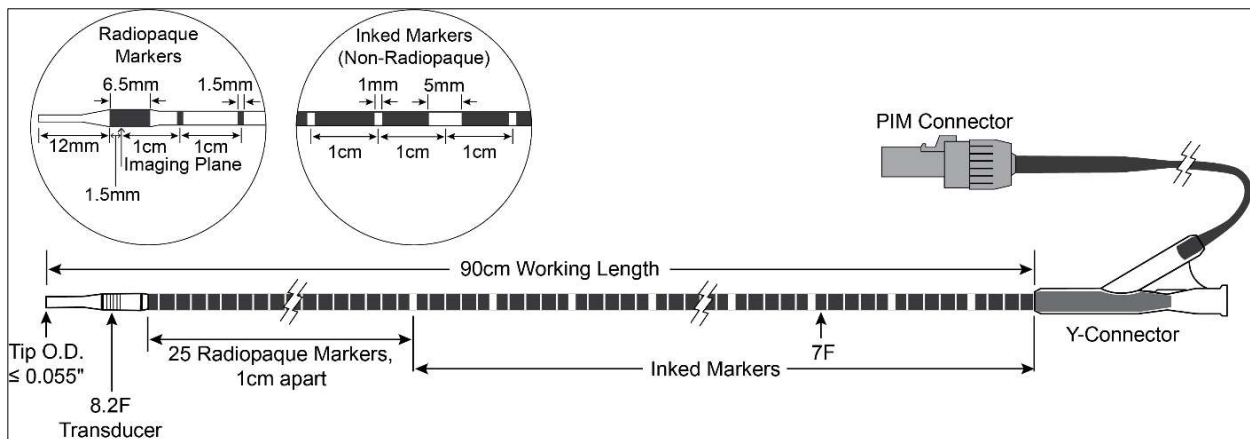


Figure 1: Visions PV .035 Catheter

A hydrophilic coating is applied externally to a distal portion of the catheter.

The Visions PV .035 catheters may only be used with Volcano s5 Series, CORE Series, and IntraSight Series of Systems. This catheter will not operate if connected to any other imaging system.

## **Instructions for Use: Reprocessed Digital IVUS Catheter**

### **INDICATIONS FOR USE**

The Reprocessed Visions PV .035 catheter is designed for use in the evaluation of vascular morphology in blood vessels of the peripheral vasculature by providing a cross-sectional image of such vessels. The Reprocessed Visions PV .035 ultrasound imaging catheter is designed for use as an adjunct to conventional angiographic procedures to provide an image of the vessel lumen and wall structures and dimensional measurements from the image.

### **CONTRAINDICATIONS FOR USE**

The Reprocessed Visions PV .035 Digital IVUS catheters are generally contraindicated in situations presenting a reasonable probability of tissue or organ damage. This device is not currently indicated for use in cerebral vessels.

- Vessel spasm
- Severe calcification
- Severe vessel tortuosity
- The catheter should not be used in patients unable to receive heparin or an acceptable alternative to achieve the adequate anticoagulation.

### **WARNINGS**

- Use of the catheter should be restricted to specialists who are familiar with, and have been trained to perform, the procedures for which this device is intended.
- The catheter transducer is a delicate electronic assembly. Deliberate misuse by bending, twisting, or any other severe manipulation may result in device malfunction.
- Do not use the device for other purposes other than those indicated.
- Tactile feedback of reprocessed devices may vary during use.

### **PRECAUTIONS**

- Do not attempt to operate the catheter prior to completely reading and understanding these directions for use.
- Protect the catheter tip from impact and excessive force.
- Do not cut, crease, knot or otherwise damage the catheter.
- Protect the electrical connections from exposure to fluid.
- Do not handle the transducer.
- The outside diameter along the entire length of the guide wire should not exceed the maximum specified.
- During use, ensure the placement of the catheter does not preclude blood flow through the vessel.
- Clean guide wire and flush catheter thoroughly with sterile heparinized normal saline before and after each insertion.
- Keep the exterior of the catheter wiped down with sterile heparinized normal saline during prolonged use.
- When inserting the guide wire both catheter and wire must be straight with no bends or kinks, or damage to inner lumen may occur.
- Do not advance the guidewire against significant resistance. If binding occurs between the catheter and the guidewire while inside the patient, CAREFULLY remove both the wire and the catheter and do not use. If binding occurs outside the patient, remove the catheter and do not use.
- When advancing or re-advancing the catheter over a guide wire and through a stented vessel, in the event that the stent is not fully apposed against the vessel wall, the guide wire/ and or catheter may become entangled in the stent between the junction of the catheter and guide wire or within one or more stent struts. This may result in entrapment of catheter/guide wire, catheter tip separation, and/or stent dislocation. Never use force to advance the catheter.
- Use caution when re-advancing a catheter over a guide wire and into a stented vessel, in the event that the catheter may come in contact with one or more stents struts. Subsequent advancement of the IVUS catheter could cause entanglement between the catheter and the

## **Instructions for Use: Reprocessed Digital IVUS Catheter**

stent(s) resulting in entrapment of catheter/ guide wire, catheter tip separation, and/or stent dislocation.

- Use caution when removing the catheter over the guide wire from a stented vessel to minimize patient risk.
- The catheter should never be forcibly inserted into lumens narrower than the catheter body or forced through a tight stenosis.
- If resistance is encountered during pullback, remove the entire system (guide wire, IVUS catheter, sheath/guide catheter) at the same time.
- Store in a cool, dark, dry place

### **ADVERSE REACTIONS**

As with all catheterization procedures, complications may be encountered with use of the catheter. Possible adverse effects include, but are not limited to, the following: occlusion; vessel spasm; vessel dissection; perforation; rupture or injury; restenosis; hemorrhage or hematoma; drug reactions; allergic reaction to contrast medium; hypo/hypertension; infection; arteriovenous fistula; embolism; entry puncture site bleeding; vascular wall injury; vessel thrombosis; pseudoaneurysm (at site of catheter insertion); renal failure; aneurysm; vessel trauma requiring surgical repair or intervention; death.

### **DIRECTIONS**

- The package label is detachable and may be affixed to the medical record of the patient.
- Inspect the catheter and packaging before opening. The contents of the package are sterile unless the package is opened or damaged. If the catheter is damaged or if the package is compromised, do not use the catheter. Return the catheter to Innovative Health. **Do not attempt to resterilize.**
- The catheter may be introduced into the vascular system percutaneously or surgically and advanced to the desired location. The frequency and duration of administration is subject to the discretion of the physician and depends upon the procedure and information required.
- Review the Volcano Imaging System Operator's Manual thoroughly prior to use of this device. Check system operation prior to the use.
- Open the catheter packaging using sterile technique and place the hoop in the sterile field.
- Prepare the catheter by flushing the guide wire lumen through the port at the catheters Y-connector, and then wipe down the entire working length with sterile heparinized normal saline.
- Connect the PIM connector of the catheter to the patient Interface Module as described in the imaging system Operator's Manual. Verify that the device is imaging.
- Place the catheter onto the intravascular guide wire. A guide wire of 0.035" (0.89 mm)-0.038" (0.97 mm) can be used).
- Activate the hydrophilic coating using the sterile heparinized normal saline.
- Advance the catheter over the guide wire to the site of the vasculature to be imaged. The guide wire should always be advanced ahead of the IVUS catheter.
- Check the Monitor for an image. Once the image has been obtained, the catheter can be advanced over the guide wire to image additional segments of vasculature.
- If an image is not obtained or not satisfactory, consult the Volcano Imaging System Operator's Manual.
- Once imaging has been completed, remove the catheter and flush thoroughly with sterile heparinized normal saline.
- For subsequent imaging, clean guide wire and flush catheter thoroughly with sterile heparinized normal saline before re-insertion.
- When the procedure is completed, remove the catheter and return the device per Innovative Health's Instructions.

**Instructions for Use: Reprocessed Digital IVUS Catheter**

**PRODUCT SPECIFICATIONS:**

|                               |                        |
|-------------------------------|------------------------|
| Model:                        | Visions PV .035        |
| Maximum shaft outer diameter: | 7.0F (0.092", 2.33mm)  |
| Maximum scanner diameter:     | 8.2F (0.108", 2.73mm)  |
| Maximum guide wire            | 0.038"(0.97 mm)        |
| Minimum Introducer Sheath     | 8.5F (0.111", 2.83 mm) |
| Usable Length                 | 90 cm                  |

| Acoustic Output Parameter     | B-Mode                |
|-------------------------------|-----------------------|
| ISPTA.3 (mW/cm <sup>2</sup> ) | 0.0534                |
| ISPPA.3 (W/cm <sup>2</sup> )  | 0.0680                |
| Pr.3 (MPa)                    | 0.0482                |
| PD (μs)                       | 0.333                 |
| PRF (Hz)                      | 2.09x10 <sup>4</sup>  |
| Center Freq (MHz)             | 9.00                  |
| MI*                           | 0.0162                |
| TI*                           | 6.18x10 <sup>-5</sup> |

Maximum overall uncertainty ±20.4%

\*As estimated tissue

**TI:** Thermal Index defined as  $TI = \frac{W_{01x1}f_c}{210}$

W<sub>01x1</sub>: Bounded-square Output (mW)

f<sub>c</sub>: Center Frequency (MHz)

MI: Mechanical Index defined as  $MI = Pr.3 / (f_c^{1/2})$

ISPPA.3: Derated Intensity, Spatial Peak Pulse Average (W/cm<sup>2</sup>)

ISPTA.3: Derated Intensity, Spatial Peak Temporal Average (mW/cm<sup>2</sup>)
















Pr.3: Derated Peak Negative Pressure at a location of the maximum derated pulse intensity integral (MPa)

PD: Pulse Duration (μs)

PRF: Pulse Repetition Frequency (Hz)

**Instructions for Use: Reprocessed Digital IVUS Catheter**

**EXPLANATION OF SYMBOLS**

|   |  |
|---|--|
|    | Federal Law in the USA restricts this device to sale by or on the order of a physician |
|    | Sterilized by Ethylene Oxide Gas   |
|    | Catalog Number   |
|    | Serial Number  |
|    | Lot Number   |
|    | Use by Date  |
|    | Do Not Reuse   |
|    | Do Not Resterilize   |
|    | Consult Instructions for Use   |
|    | Keep Product Dry   |
|    | Manufacturer   |
|    | Keep Away from Sunlight  |
|    | Do Not Use if Package is Damaged   |
|   | Non-pyrogenic  |
|  | Not made with Natural Rubber Latex   |

As the reprocessor, Innovative Health is solely responsible for this device. All Original Manufacturer (OM) information is provided for device identification and may contain trademarks from third parties that do not sponsor this device.

**Sterilization:** This product and its packaging have been sterilized with ethylene oxide (EO) gas. Even though the product is processed in compliance with all applicable laws and regulations relating to EO exposure, Proposition 65, a State of California voter initiative, requires the following notice:

**Warning:** This product and its packaging have been sterilized with EO. The packaging may expose you to EO, a chemical known to the State of California to cause cancer or birth defects or other reproductive harm.

Visions and Volcano are registered trademarks of Volcano Corporation.

Please refer to [www.innovative-health.com](http://www.innovative-health.com) for product warranty.